



# **15-EPI-LIPOXIN A<sub>4</sub> ELISA Kit Instructions**

**Please read all instructions carefully before beginning this assay**

PRODUCT #407110

For Research Use Only

**Storage Conditions:**  
**Lyophilized conjugate: -20°C or less**  
**Do not freeze reconstituted conjugate**  
**All other kit components: 2-8°C**

## **DESCRIPTION**

15-epi-Lipoxin A<sub>4</sub> is an aspirin-triggered eicosanoid believed to be involved in the positive attributes of aspirin therapy for heart, cancer, and human immunodeficiency virus patients. During inflammation, neutrophils are activated. 15-epi-LXA<sub>4</sub>, when administered *in vivo*, inhibits neutrophil activation and dampens inflammation (Takano, 1997). 15-epi-LXA<sub>4</sub> is naturally formed in the body via this pathway:

Arachidonic Acid (AA) → 15(R)-HETE → 15-epi-LXA<sub>4</sub>

Aspirin is thought to be involved in the acetylation of prostaglandin G/H synthase, which triggers the conversion of AA to 15(R)-HETE.


The development of this assay, which is both sensitive and selective for 15-epi-LXA<sub>4</sub>, will be essential to researchers studying anti-inflammatory medications.

## **PRINCIPLE OF ASSAY**

This is an ELISA (Enzyme-Linked ImmunoSorbent Assay) for the quantitative analysis of 15-epi-Lipoxin A<sub>4</sub> levels in biological fluid. This test kit operates on the basis of competition between the enzyme conjugate and 15-epi-Lipoxin A<sub>4</sub> in the sample for a limited number of binding sites.

First, the sample or standard solution is added to the microplate. Next, the diluted enzyme conjugate is added and the mixture is shaken and incubated at room temperature for one hour. During the incubation, competition for binding sites is taking place. The plate is then washed, removing all the unbound material. The bound enzyme conjugate is detected by the addition of substrate which generates an optimal color after 30 minutes. Quantitative test results may be obtained by measuring and comparing the absorbance reading of the wells of the samples against the standards with a microplate reader at 650 nm. The extent of color development is inversely proportional to the amount of 15-epi-Lipoxin A<sub>4</sub> in the sample or standard. For example, the absence of 15-epi-Lipoxin A<sub>4</sub> in the sample will result in a bright blue color, whereas the presence of 15-epi-Lipoxin A<sub>4</sub> will result in decreased or no color development.

## PRINCIPLE OF ASSAY (continued)

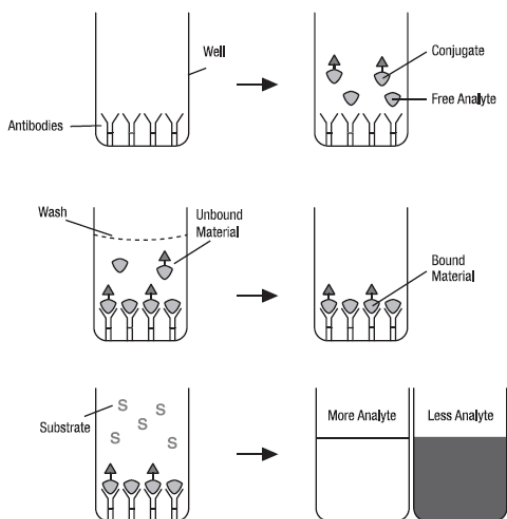

## MATERIALS PROVIDED

1. **EIA BUFFER:** 30 mL. Provided to dilute enzyme conjugate and 15-epi-Lipoxin  $A_4$  standards.
2. **WASH BUFFER (10X):** 20 mL. Dilute 10-fold with deionized water. Diluted wash buffer is used to wash all unbound enzyme conjugate, sample and standards from the plate after the one hour incubation.
3. **K-BLUE SUBSTRATE:** 20 mL. Stabilized 3,3', 5,5' Tetramethylbenzidine (TMB) plus Hydrogen Peroxide ( $H_2O_2$ ) in a single bottle. It is used to develop the color in the wells after the wash step. **LIGHT SENSITIVE.** Keep substrate refrigerated.
4. **EXTRACTION BUFFER (5X):** 30mL. Dilute 5-fold with deionized water. This is used for diluting extracted and non-extracted samples.
5. **15-epi-Lipoxin  $A_4$  ENZYME LYOPHILIZED CONJUGATE:** Two vials of lyophilized 15-epi-LXA $_4$  horse-radish peroxidase conjugate. Reconstitution with 75  $\mu$ L of deionized water results in a 50:1 concentrate. Blue capped vials.
6. **15-epi-Lipoxin  $A_4$  STANDARD:** 100  $\mu$ L. 15-epi-Lipoxin  $A_4$  standard at the concentration of 1  $\mu$ g/mL. Green capped vial.
7. **15-epi-Lipoxin  $A_4$  ANTIBODY COATED PLATE:** A 96 well Costar® microplate with anti-15-epi-LXA $_4$  rabbit antibody precoated on each well. The plate is ready to use as is.

**DO NOT WASH.**

## MATERIALS NEEDED BUT NOT PROVIDED

1. 300 mL deionized water for diluting wash buffer, extraction buffer and lyophilized conjugate.
2. Precision pipettes that range from 10  $\mu$ L - 1000  $\mu$ L and disposable tips.

**NOTE:** *If all or several strips are to be used at one time, it is suggested that a multichannel pipette be used.*

3. Clean test tubes used to dilute the standards and conjugate.
4. Graduated cylinder to dilute and mix wash buffer and extraction buffer.
5. Microplate reader with 650 nm filter.
6. Plate cover or plastic film to cover plate during incubation.

## OPTIONAL MATERIALS:

- 1 N HCl or Neogen's Red Stop Solution.
- Microplate shaker.

If performing an extraction on samples, the following will be required:

- 1N HCl
- Hexane
- C<sub>18</sub> Sep-Pak® light column (Waters® Corporation)
- Methyl formate
- Methanol
- Nitrogen gas
- Centrifuge

## WARNINGS AND PRECAUTIONS

- DO NOT** use components beyond expiration date.
- DO NOT** mix any reagents or components of this kit with any reagents or components of any other kit. This kit is designed to work properly as provided.
- DO NOT** pipette reagents by mouth.
- Always pour substrate out of the bottle into a clean test tube. **DO NOT** pipette out of the bottle. If the pipette tip is unclean, this could result in contamination of the substrate.
- All specimens should be considered potentially infectious. Exercise proper handling precautions.
- DO NOT** smoke, eat or drink in areas where specimens or reagents are being handled.
- Use aseptic technique when opening and removing reagents from vials and bottles.
- Keep plate covered except when adding reagents, washing or reading.
- Kit components should be refrigerated at all times when not in use; lyophilized conjugate, frozen.
- Ensure that the conjugate is completely reconstituted before use. Each vial, when reconstituted, provides sufficient reagent to perform 64 assays (8 strips). If more than 64 assays are to be run, reconstitute both vials and pool the reconstituted conjugate.

## PROCEDURAL NOTES

- It is not necessary to allow reagents to warm to room temperature before use.
- Desiccant bag must remain in foil pouch with unused strips. Keep zip-lock pouch sealed when not in use to maintain a dry environment.
- Always use clean pipette tips for the buffer, enzyme conjugate, standards and samples.
- Before pipetting a reagent, rinse the pipette tip three times with that reagent (i.e. fill the tip with the desired amount of reagent and dispense back into the same vial - repeat 2 times). Now the tip is properly rinsed and ready to dispense the reagent into your well or test tube.
- When pipetting into the wells, **DO NOT** allow the pipette tip to touch the inside of the well, or any of the reagents already in the well. This can result in cross contamination.
- Standards and samples should be assayed in duplicate.
- To quantitate, always run samples alongside a standard curve. If testing a sample that is not extracted, standards should be diluted in the same type of medium being tested. This medium should be known to be negative.
- Gently mix specimens and reagents before use. Avoid vigorous agitation.
- Before opening the lyophilized conjugate vial, examine the vial to ensure that lyophilized material has not been trapped in the cap. If material is in the cap, gently tap the upright vial to dislodge the trapped material.
- To reconstitute the lyophilized conjugate, add 75  $\mu$ L of deionized water to a vial. Rehydrate the conjugate by gently rotating the vial. Do not vortex or shake the contents. Avoid excess foaming. After the solid material has gone into solution, the conjugate is ready to be diluted. Write the date of reconstitution on the label. Concentrated, reconstituted conjugate has a shelf life of at least two weeks when stored at 2-8°C.
- The enzyme conjugate is most stable in its concentrated form. Dilute only the volume necessary for the amount of strips currently being used.
- Before taking an absorbance reading, wipe the outside bottom of the wells with a lint-free wiper to remove dust and fingerprints.

## SAMPLE PREPARATION

This assay is non-species specific. Usually, urine and tissue culture supernatant can be assayed directly by diluting them with the diluted extraction buffer. Dilute specimens may require extraction in order to concentrate 15-epi-LXA<sub>4</sub>. Plasma and most other mediums will require extraction. Listed below is one possible extraction method.

### EXTRACTION OF 15-EPI LIPOXIN A<sub>4</sub>

1. Dilute 100 µL sample with 200 µL of methanol then dilute the previous volume with 1.5 mL of water.
2. For 1 mL sample: Acidify to pH 3.5 with 1N HCl.
3. Precondition the C<sub>18</sub> Sep-Pak® light column (Waters® Corporation) by washing the column with 2 mL of methanol followed by 2 mL of water.
4. Apply the above sample into the column and wash the column with 5 mL of water followed by 5 mL of hexane.
5. Elute 15-epi-LXA<sub>4</sub> with 2 mL of methyl formate.
6. Evaporate methyl formate with a stream of N<sub>2</sub>.
7. Reconstitute the residue with 1 mL of diluted extraction buffer and assay for 15-epi Lipoxin A<sub>4</sub> content.

**NOTE: Extraction buffer must be diluted 5-fold with deionized water before use. Any precipitant present must be brought into solution before dilution..**

## TEST PROCEDURES

1. Prepare standards as follows:

<b>Standard</b>	<b>Preparation</b>
A	stock solution 1 µg/mL (provided in green capped vial)
B	take 10 µL of A, add to 490 µL of buffer and mix=20 ng/mL
C	take 200 µL of B, add to 1.8 mL of buffer and mix=2 ng/mL
D	take 200 µL of C, add to 1.8 mL of buffer and mix=0.2 ng/mL

Continue standard preparation following Scheme I.

### SCHEME I

<b>Standards</b>	<b>ng/mL</b>	<b>EIA buffer (µL added)</b>	<b>C standard µL</b>	<b>D standard µL</b>
S <sub>0</sub>	0	as is	-	-
S <sub>1</sub>	0.02	900	-	100
S <sub>2</sub>	0.05	750	-	250
S <sub>3</sub>	0.1	500	-	500
S <sub>4</sub>	0.2	-	-	as is
S <sub>5</sub>	0.5	750	250	-
S <sub>6</sub>	1	500	500	-
S <sub>7</sub>	2	-	as is	-

2. Determine the number of wells to be used.
3. Dilute the reconstituted 15-epi-Lipoxin A<sub>4</sub> enzyme conjugate. Add 1 µL of conjugate to 50 µL total volume of EIA buffer for each well assayed. For the entire plate, add 110 µL of the 15-epi-Lipoxin A<sub>4</sub> enzyme conjugate into 5.5 mL total volume of EIA buffer. Mix the solution thoroughly.

**NOTE: If more concentrated conjugate is needed than is contained in the first conjugate vial, reconstitute and use the second vial. Do not use the separate contents of both vials in the same assay as some assay variability may result. If the contents of both vials are required for an assay, pool the concentrated conjugates. Use the expiration date of the**

**oldest reconstituted vial for the pool. Alternatively, prepare the necessary volumes of diluted conjugate and pool before using in the assay.**

- Add 50  $\mu\text{L}$  of standard (S) or unknown (U) (some samples may require diluting) to the appropriate wells in duplicate.

**See Scheme II for suggested template design.**

- Add 50  $\mu\text{L}$  of the diluted enzyme conjugate to each well. Use 8-channel pipette or 12-channel pipette for rapid addition.
- Mix by shaking plate gently. A microplate shaker may be used.
- Cover plate with plastic film or plate cover and incubate at room temperature for one hour.

**NOTE: Keep plate away from drafts and temperature fluctuations.**

- Dilute concentrated wash buffer with deionized water (i.e. 20 mL of wash buffer plus 180 mL of deionized water). Mix thoroughly.
- After incubation, dump out the contents of the plate. Tap out contents thoroughly on a clean lint-free towel.
- Wash each well with 300  $\mu\text{L}$  of the diluted wash buffer. Repeat for a total of three washings. An automated plate washer can be used, however, increase wash cycles from three to five.
- Add 150  $\mu\text{L}$  of substrate to each well. Use multichannel pipette for best results. Mix by shaking plate gently.
- Incubate at room temperature for 30 minutes.
- Gently shake plate before taking a reading to ensure uniform color throughout each well.
- Plate is read in a microplate reader at 650 nm. If a dual wavelength is used, set  $W_1$  at 650 nm and  $W_2$  at 490 nm.
- If accounting for substrate background, use 2 to 8 wells as blanks with only substrate in the wells (150  $\mu\text{L}$ /well). Subtract the average of these absorbance values from the absorbance values of the wells being assayed.

**NOTE: Some microplate readers can be programmed to do the background subtractions automatically when reading the plate. Consult your instrument manual.**

## OPTIONAL TEST PROCEDURES

- Add 50-100  $\mu\text{L}$  of 1 N HCl or Neogen's Red Stop Solution to each well to stop enzyme reaction.
- Read plate at 450 nm, if 1N HCl solution was used. Read plate at 650 nm, if Neogen's Red Stop Solution was used.
- Plot the standard curve and estimate the concentrations of the samples from the curve. See "CALCULATIONS."

**NOTE: Absorbance readings will approximately double when stopped with acid. If absorbance readings are too high for measuring with your microplate reader, decrease the substrate incubation approximately 10 minutes but no more than 15 minutes.**

## SCHEME II

	1	2	3	4	5	6	7	8	9	10	11	12
A	$S_0$	$S_0$	$U_1$	$U_1$	$U_9$	$U_9$	$U_{17}$	$U_{17}$	$U_{25}$	$U_{25}$	$U_{33}$	$U_{33}$
B	$S_1$	$S_1$	$U_2$	$U_2$	$U_{10}$	$U_{10}$	$U_{18}$	$U_{18}$	$U_{26}$	$U_{26}$	$U_{34}$	$U_{34}$
C	$S_2$	$S_2$	$U_3$	$U_3$	$U_{11}$	$U_{11}$	$U_{19}$	$U_{19}$	$U_{27}$	$U_{27}$	$U_{35}$	$U_{35}$
D	$S_3$	$S_3$	$U_4$	$U_4$	$U_{12}$	$U_{12}$	$U_{20}$	$U_{20}$	$U_{28}$	$U_{28}$	$U_{36}$	$U_{36}$
E	$S_4$	$S_4$	$U_5$	$U_5$	$U_{13}$	$U_{13}$	$U_{21}$	$U_{21}$	$U_{29}$	$U_{29}$	$U_{37}$	$U_{37}$
F	$S_5$	$S_5$	$U_6$	$U_6$	$U_{14}$	$U_{14}$	$U_{22}$	$U_{22}$	$U_{30}$	$U_{30}$	$U_{38}$	$U_{38}$
G	$S_6$	$S_6$	$U_7$	$U_7$	$U_{15}$	$U_{15}$	$U_{23}$	$U_{23}$	$U_{31}$	$U_{31}$	$U_{39}$	$U_{39}$
H	$S_7$	$S_7$	$U_8$	$U_8$	$U_{16}$	$U_{16}$	$U_{24}$	$U_{24}$	$U_{32}$	$U_{32}$	$U_{40}$	$U_{40}$


## CALCULATIONS

- After the substrate background has been subtracted from all absorbance values, average all of your duplicate well absorbance values.
- The average of your two  $S_0$  values is now your  $B_0$  value. ( $S_1$  now becomes  $B_1$ , etc.)
- Next, find the percent of maximal binding (% $B/B_0$  value). To do this, divide the averages of each standard absorbance value (now known as  $B_1$  through  $B_7$ ) by the  $B_0$  absorbance value and multiply by 100 to achieve percentages.

- Graph your standard curve by plotting the  $\%B/B_0$  for each standard concentration on the ordinate (y) axis against concentration on the abscissa (x) axis. Draw a curve by using a curve-fitting routine (i.e. 4-parameter or linear regression).
- Divide the averages of each sample absorbance value by the  $B_0$  value and multiply by 100 to achieve percentages.
- Using the standard curve, the concentration of each sample can be determined by comparing the  $\%B/B_0$  of each sample to the corresponding concentration of 15-epi-Lipoxin  $A_4$  standard.
- If the samples were diluted, the concentration determined from the standard curve must be multiplied by the dilution factor.

## TYPICAL STANDARD CURVE

15-epi-Lipoxin  $A_4$  in EIA Buffer

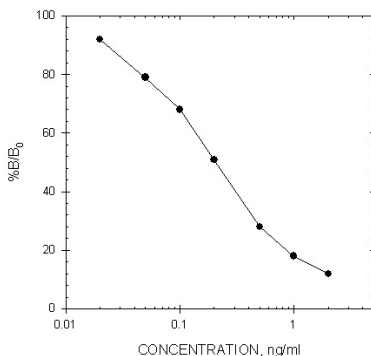

## TYPICAL DATA

**NOTE:** "Typical data" is a representation. Variances in data will occur. Optical density readings may fluctuate during the shelf-life of the kit, but the  $\%B/B_0$  should remain comparable. Measuring wavelength: 650 nm

Standard	Standard Concentration (ng/mL)	Optical Density (Absorbance Value)	$\%B/B_0$
$S_0 (B_0)$	0	1.057	100
$S_1 (B_1)$	0.02	0.977	92
$S_2 (B_2)$	0.05	0.833	79
$S_3 (B_3)$	0.1	0.715	68
$S_4 (B_4)$	0.2	0.539	51
$S_5 (B_5)$	0.5	0.301	28
$S_6 (B_6)$	1	0.193	18
$S_7 (B_7)$	2	0.125	12

## CROSS REACTIVITY

15-EPI-LIPOXIN <sub>4</sub> .....	100.0%
LIPOXIN $A_4$ .....	3.0%
15(R)-HETE.....	0.8%
5(S)-HETE.....	<0.01%
12(S)-HETE.....	<0.01%
15(S)-HETE.....	<0.01%

## REFERENCES

1. Chiang, N., Takano, T., Clish, C., Petasis, N., Tai, H.H., and Serhan, C. Aspirin-Triggered 15-epi-Lipoxin A4 (ATL) Generation by Human Leukocytes and Murine Peritonitis Exudates: Development of a specific 15-epi-LXA4 ELISA. *The Journal of Pharmacology and Experimental Therapeutics*. 287(2): 779-790 (1998).
2. Planaguma, A., Titos, E., Lopez-Parra, M., Gaya, J., Pueyo, G., Arroyo, V., and Claria, J. Aspirin (ASA) regulates 5-lipoxygenase activity and peroxisome proliferators-activated receptor  $\alpha$ -mediated CINC-1 release in rat liver cells: novel actions of lipoxin A4 (LXA4) and ASSA-triggered 15-epi-LXA4. *The FASEB Journal*. 1937-1939 (2002).
3. Serhan, C.N., Takano, T., and Maddox, J.F. Aspirin-triggered 15-epi-lipoxin A4 and stable analogs of lipoxin A4 are potent inhibitors of acute inflammation. In *Lipoxygenases and Their Metabolites*, S. Nigam, C.R. Pace-Asciak, Eds., Kluwer Academic Press, 1999, pp. 133-149.
4. Serhan, C.N. Lipoxins and Novel Aspirin-triggered 15-epi-Lipoxins (ATL): A Jungle of Cell-Cell Interactions or a Therapeutic Opportunity. *Prostaglandins*. 53: 107-137 (1997).
5. Takano, T., Fiore, S., Maddox, J.F., Brady, H.R., Petasis, N.A. and Serhan, C.N. Aspirin-triggered 15-epi-lipoxinA4 (LXA4) and LXA4 stable analogues are potent inhibitors of acute inflammation: evidence for anti-inflammatory receptors. *J. Exp. Med.* 185(9): 1693-1704 (1997).
6. Takano, T., Clish, C.B., Gronert, K., Petasis, N., and Serhan, C.N. Neutrophil-mediated changes in vascular permeability are inhibited by topical applications of aspirin-triggered 15-epi-lipoxin A4 and novel lipoxin B4 stable analogues. *J. Clin. Invest.* 101: 819-26 (1998).

## COPYRIGHT

All rights reserved worldwide. No part of this publication may be reproduced, transmitted, transcribed, or stored in any information-retrieval system, or translated into any human or computer language in any form or by any means (manual, electronic, mechanical, magnetic, optical, chemical, or otherwise) without expressed written permission.

## WARRANTY

Neogen Corporation makes no warranty of any kind, either expressed or implied, except that the material from which its products are made are of standard quality. If any materials are defective, Neogen Corporation will provide a replacement product. Buyer assumes all risk and liability resulting from the use of this product and any of the predictive models. There is no warranty of merchantability of this product, or of the fitness of the product for any purpose. Neogen Corporation shall not be liable for any damages, including special or consequential damage, or expense arising directly or indirectly from the use of this product.

## TECHNICAL ASSISTANCE

Technical assistance is available Monday-Friday, between 8:00 a.m. and 6:00 p.m. EST.



944 Nandino Blvd • Lexington KY 40511-1205 USA  
859/254-1221 or 800/477-8201 USA/CANADA  
Fax: 859/255-5532 • email: [inform@neogen.com](mailto:inform@neogen.com)